


CONFORM

PIVOTAL TRIAL

CLAAS[®] Implant Procedure

CAUTION: Investigational device. Limited by United States
law to investigational use only. Not available for sale.

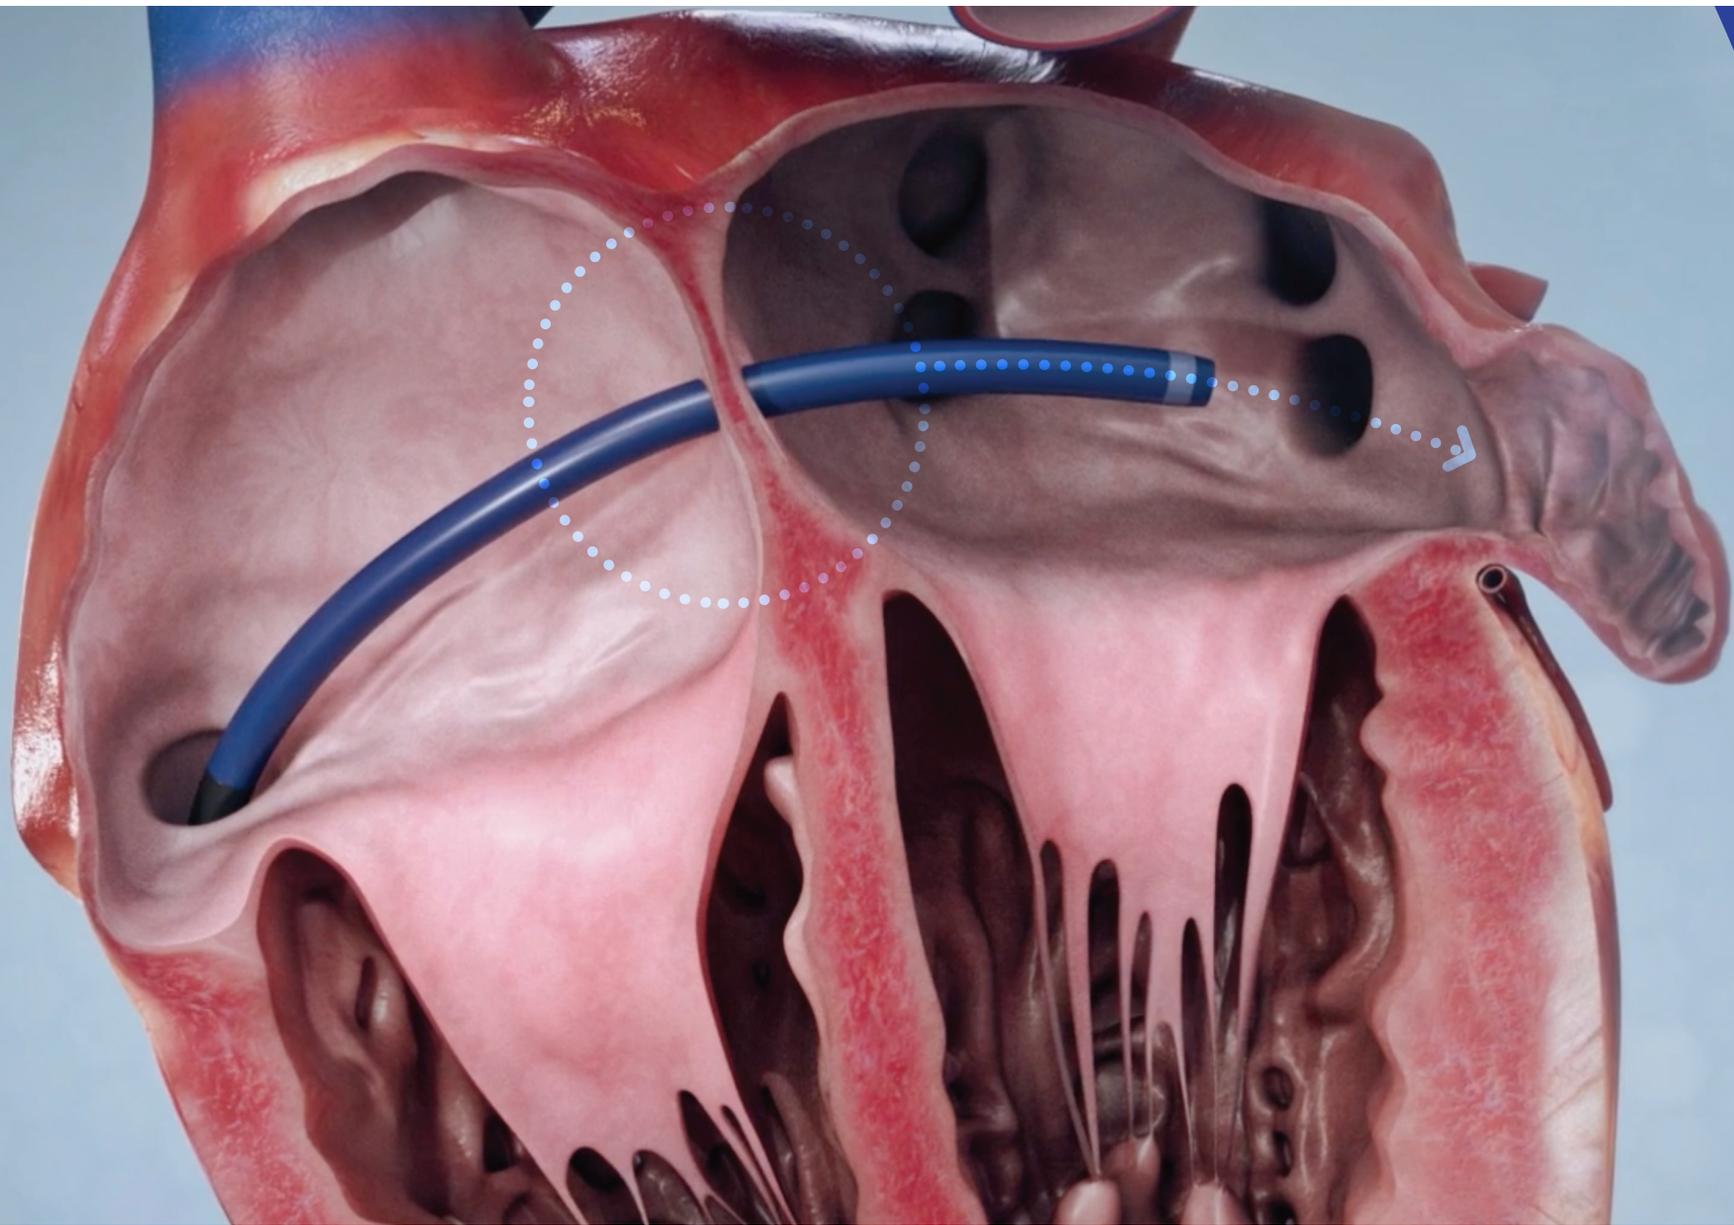


01

CONFORM
PIVOTAL TRIAL

Left Atrial Appendage Access

The catheter crosses the heart wall and enters the left atrium.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

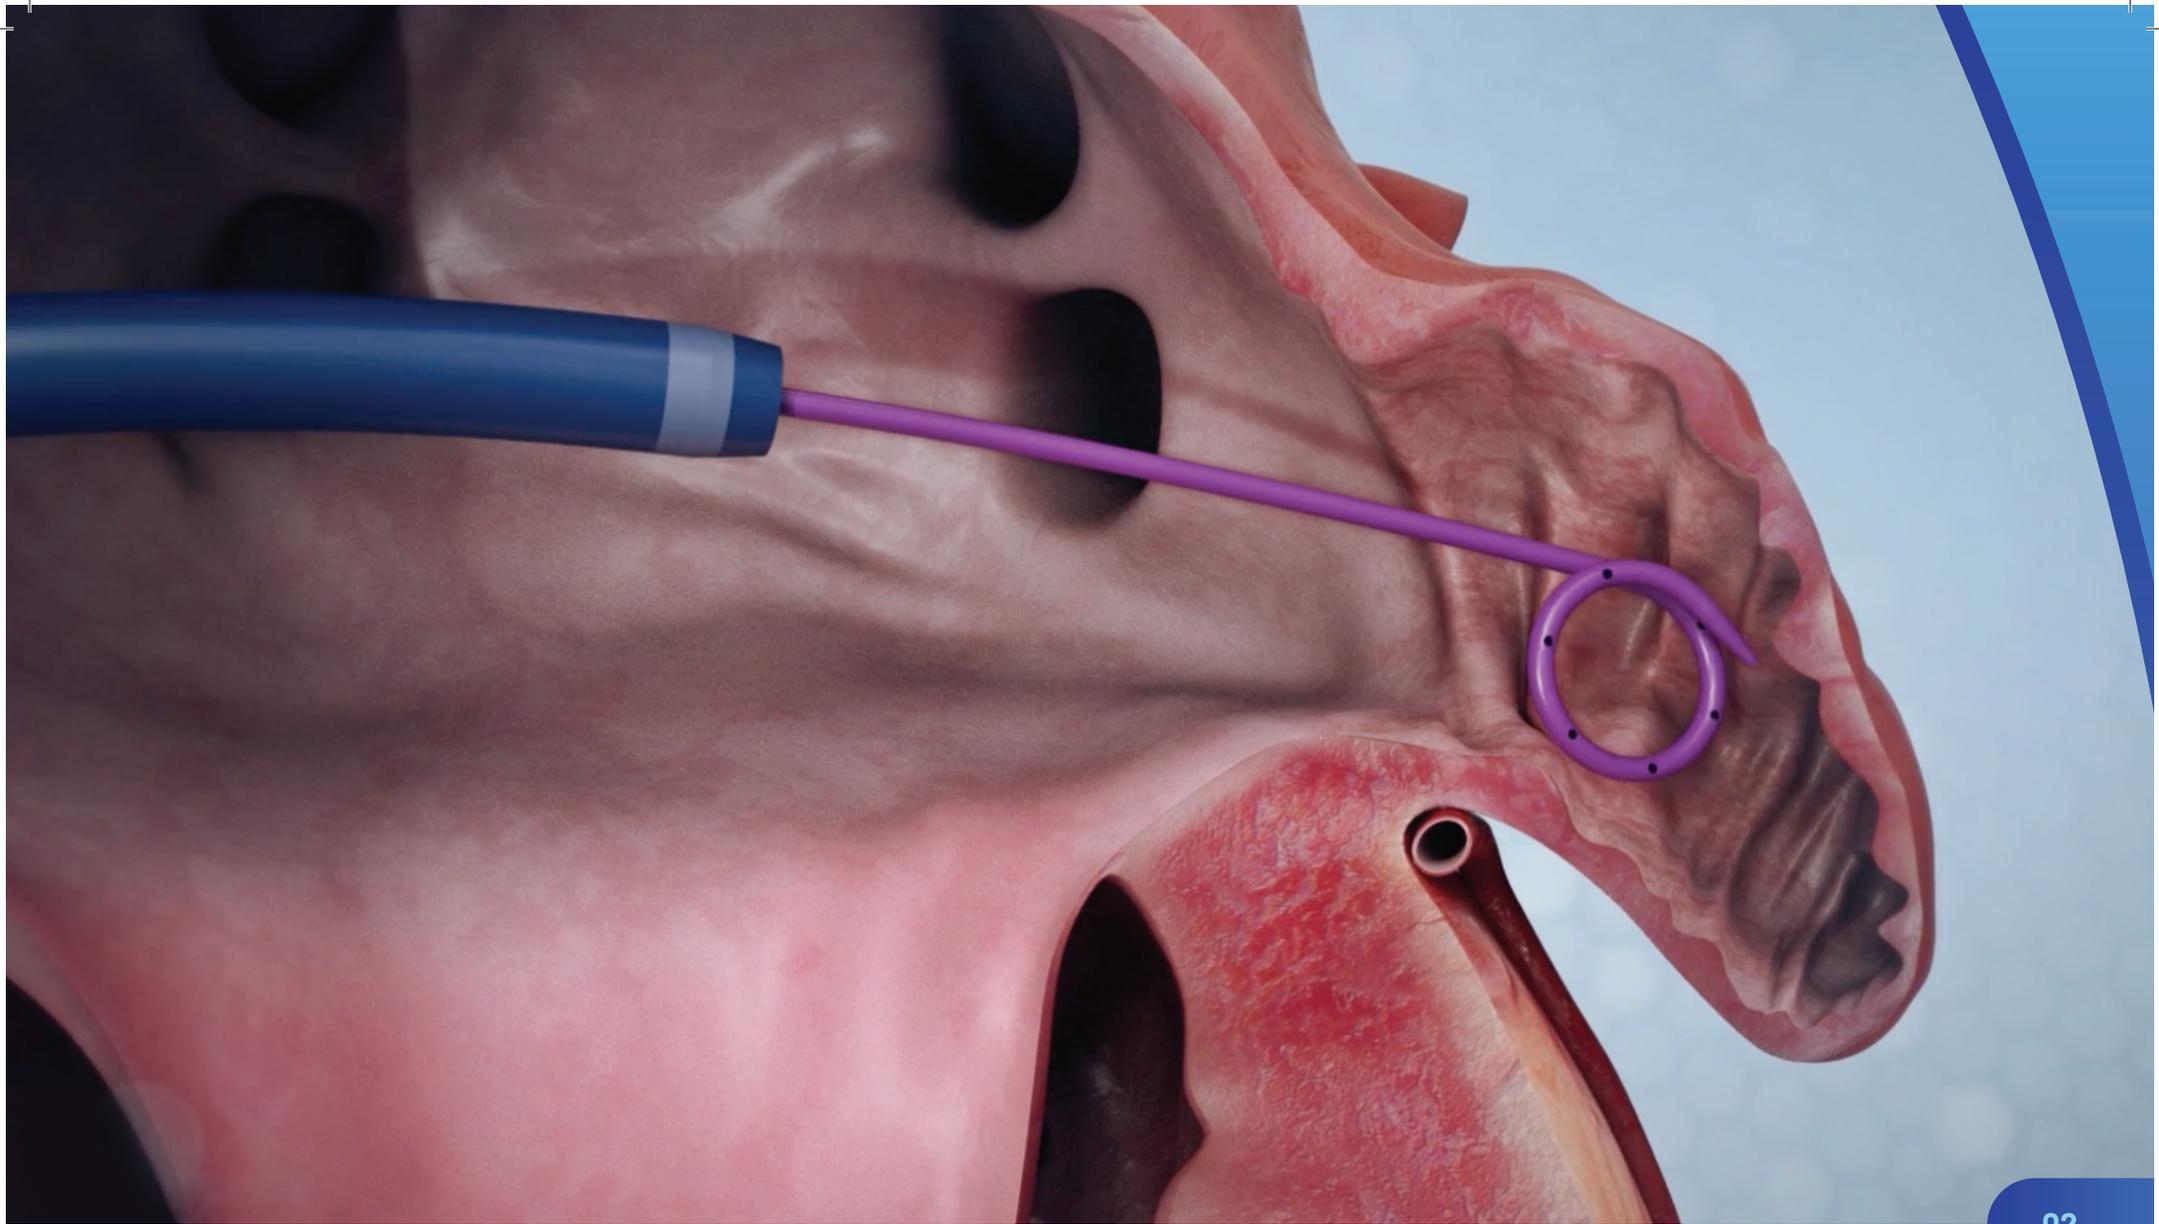


CONFORM
PIVOTAL TRIAL

Access Catheter Positioned

The catheter is placed into the appendage.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

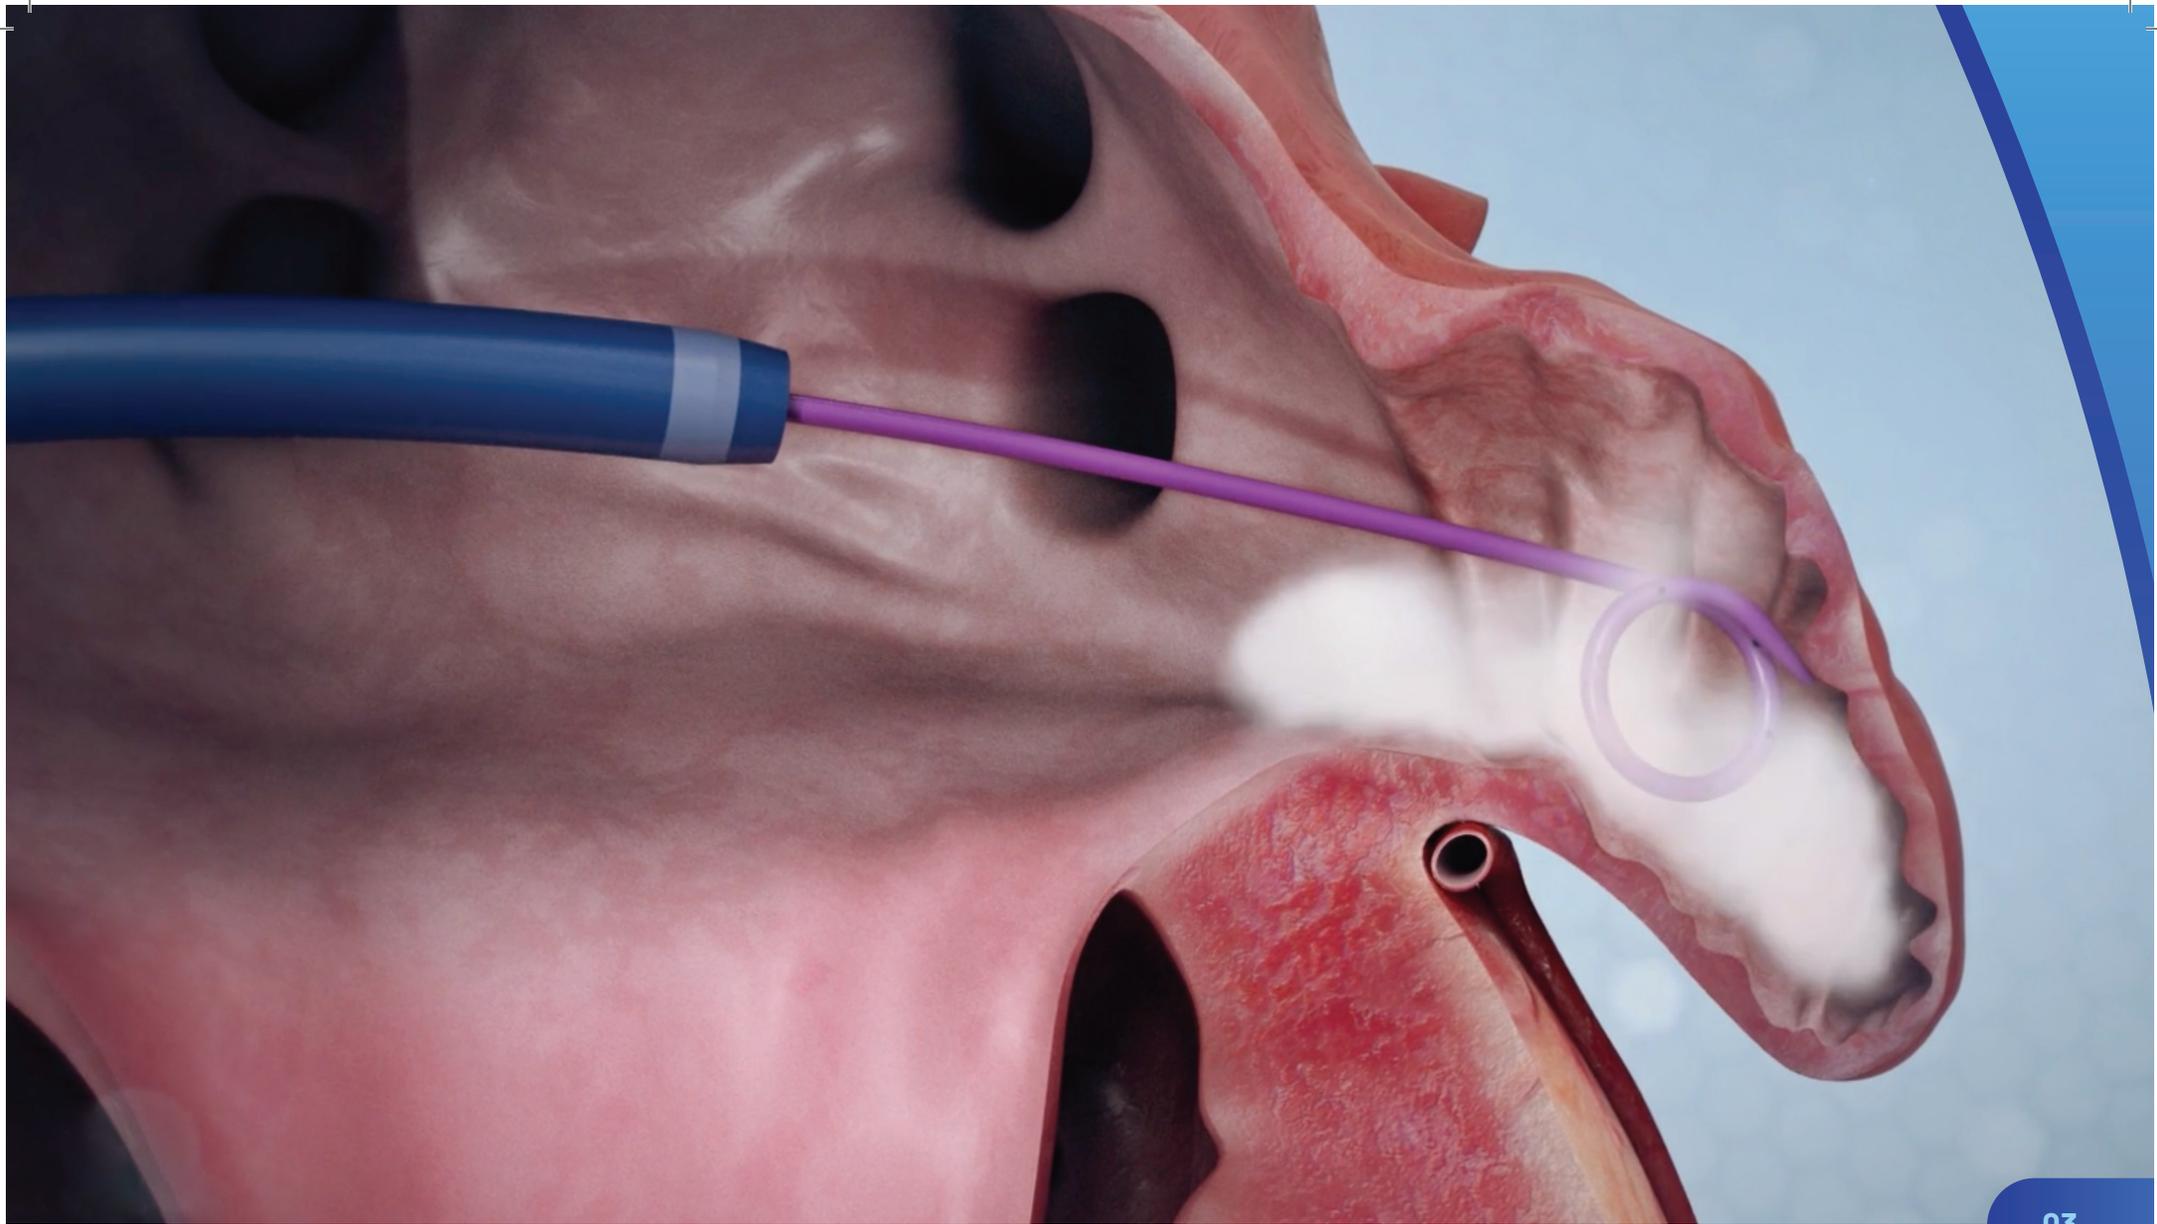


CONFORM

PIVOTAL TRIAL

Imaging

Images are taken to view and size the appendage.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

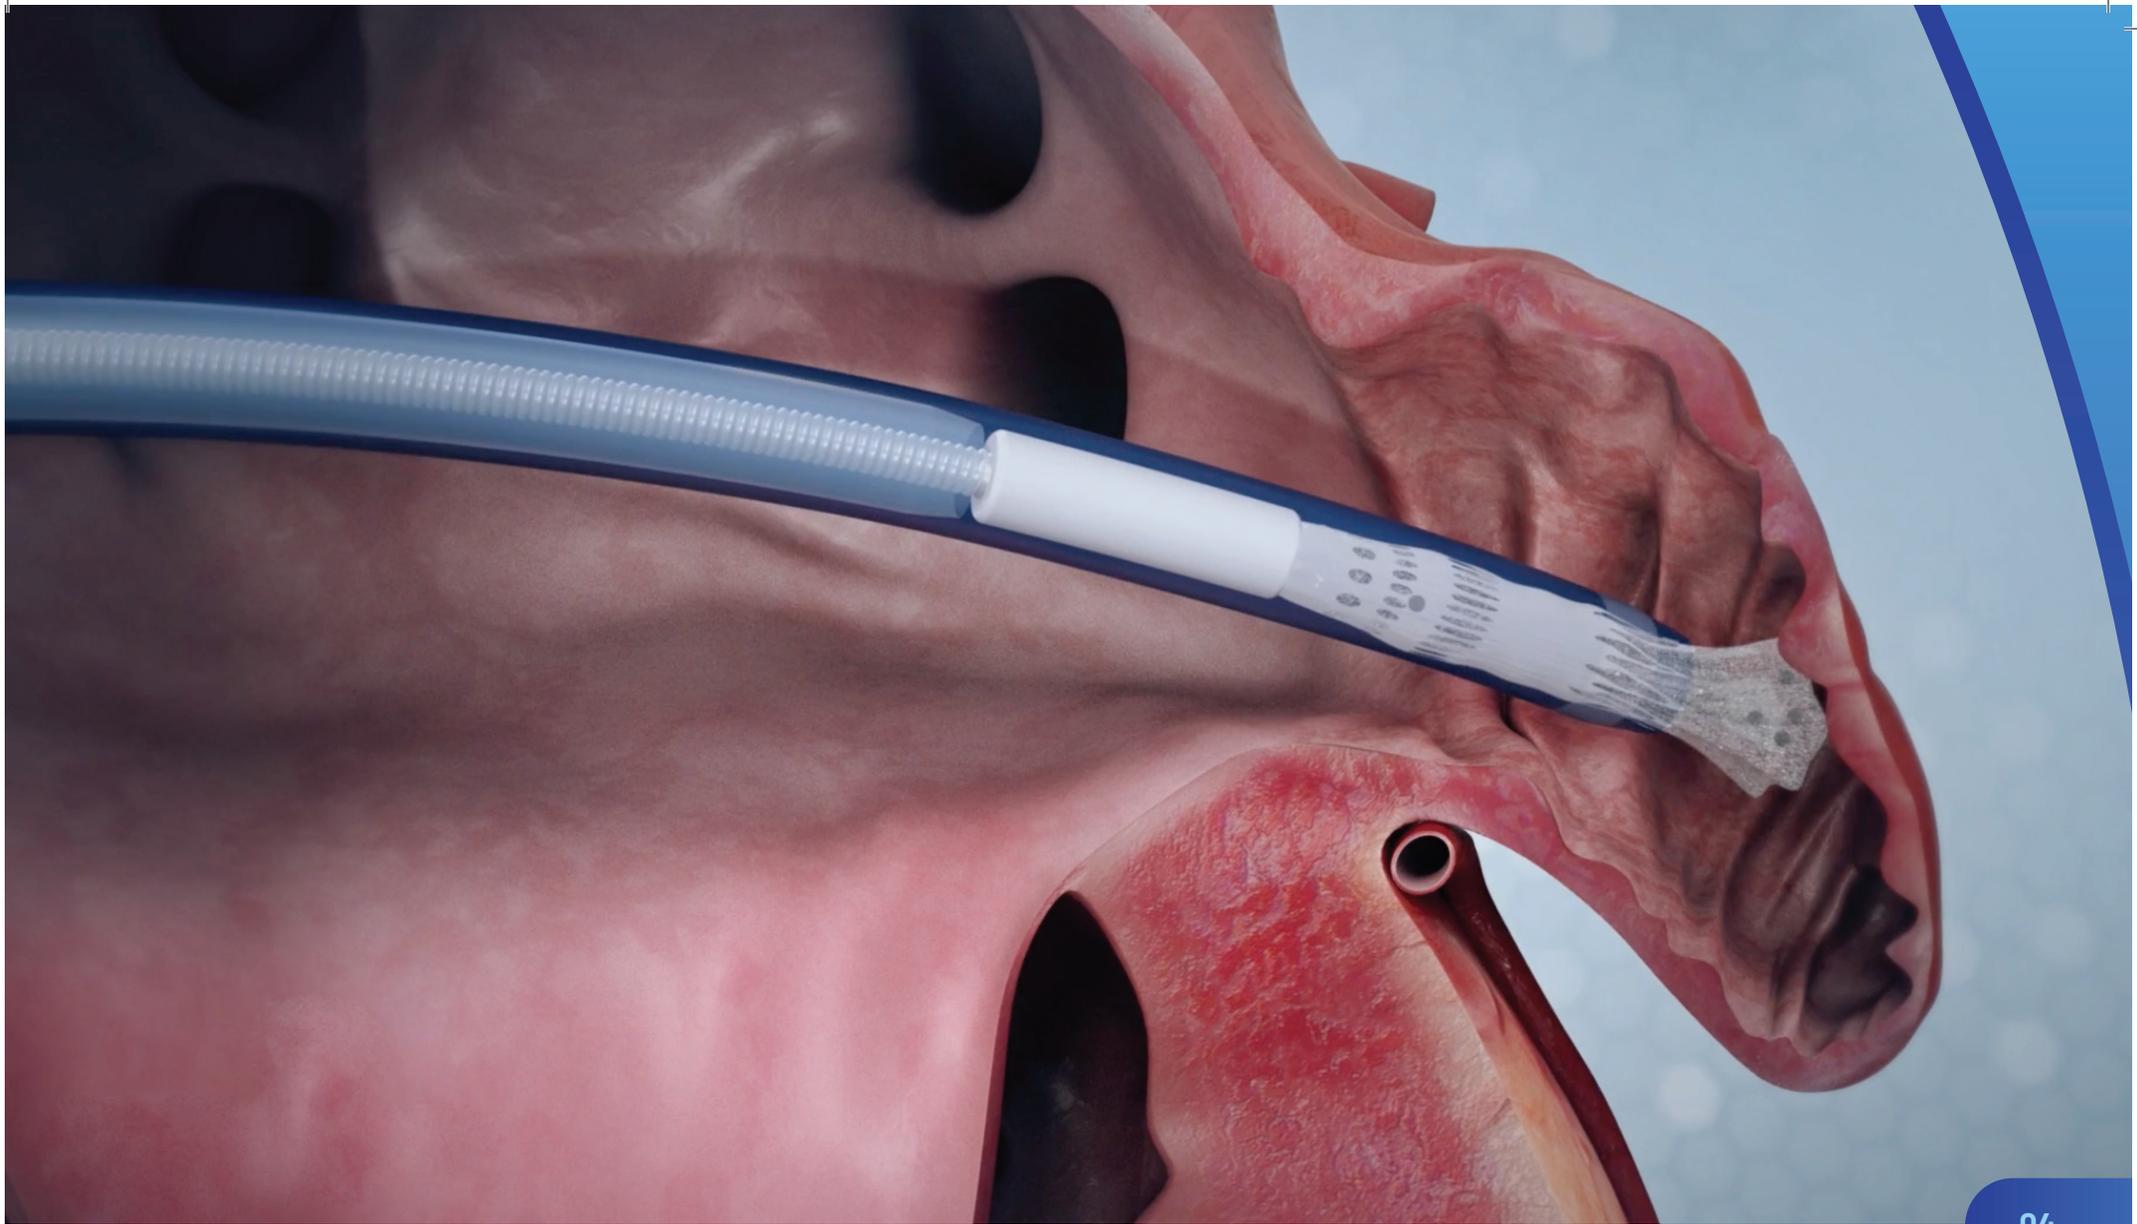


CONFORM

PIVOTAL TRIAL

Implant Positioned

The implant is delivered through the catheter and placed into the appendage.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

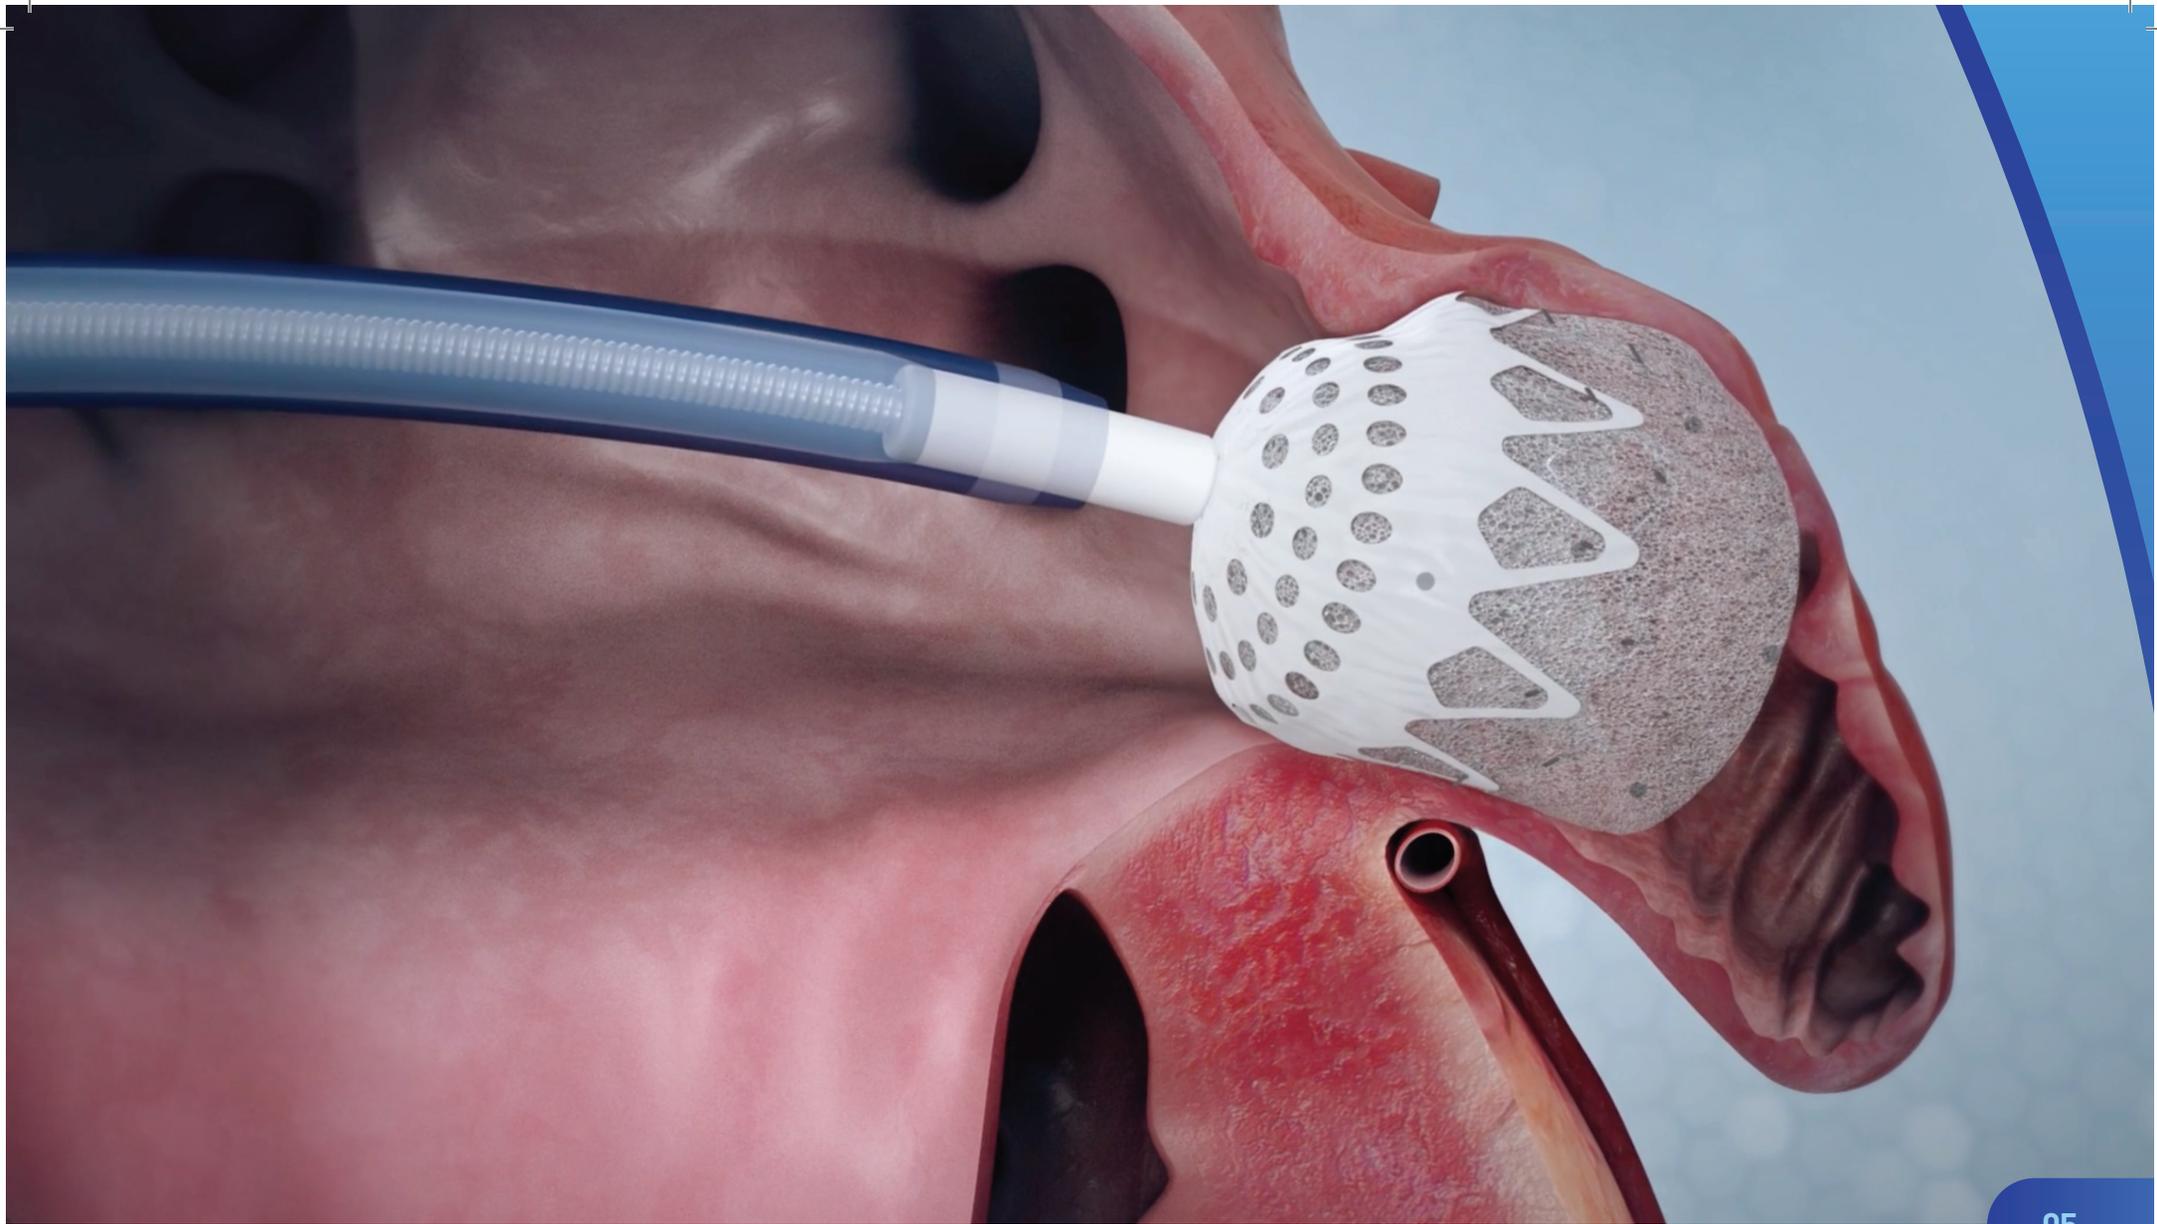


CONFORM
PIVOTAL TRIAL

Implant Deployed

Once deployed, the implant conforms to seal the appendage.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

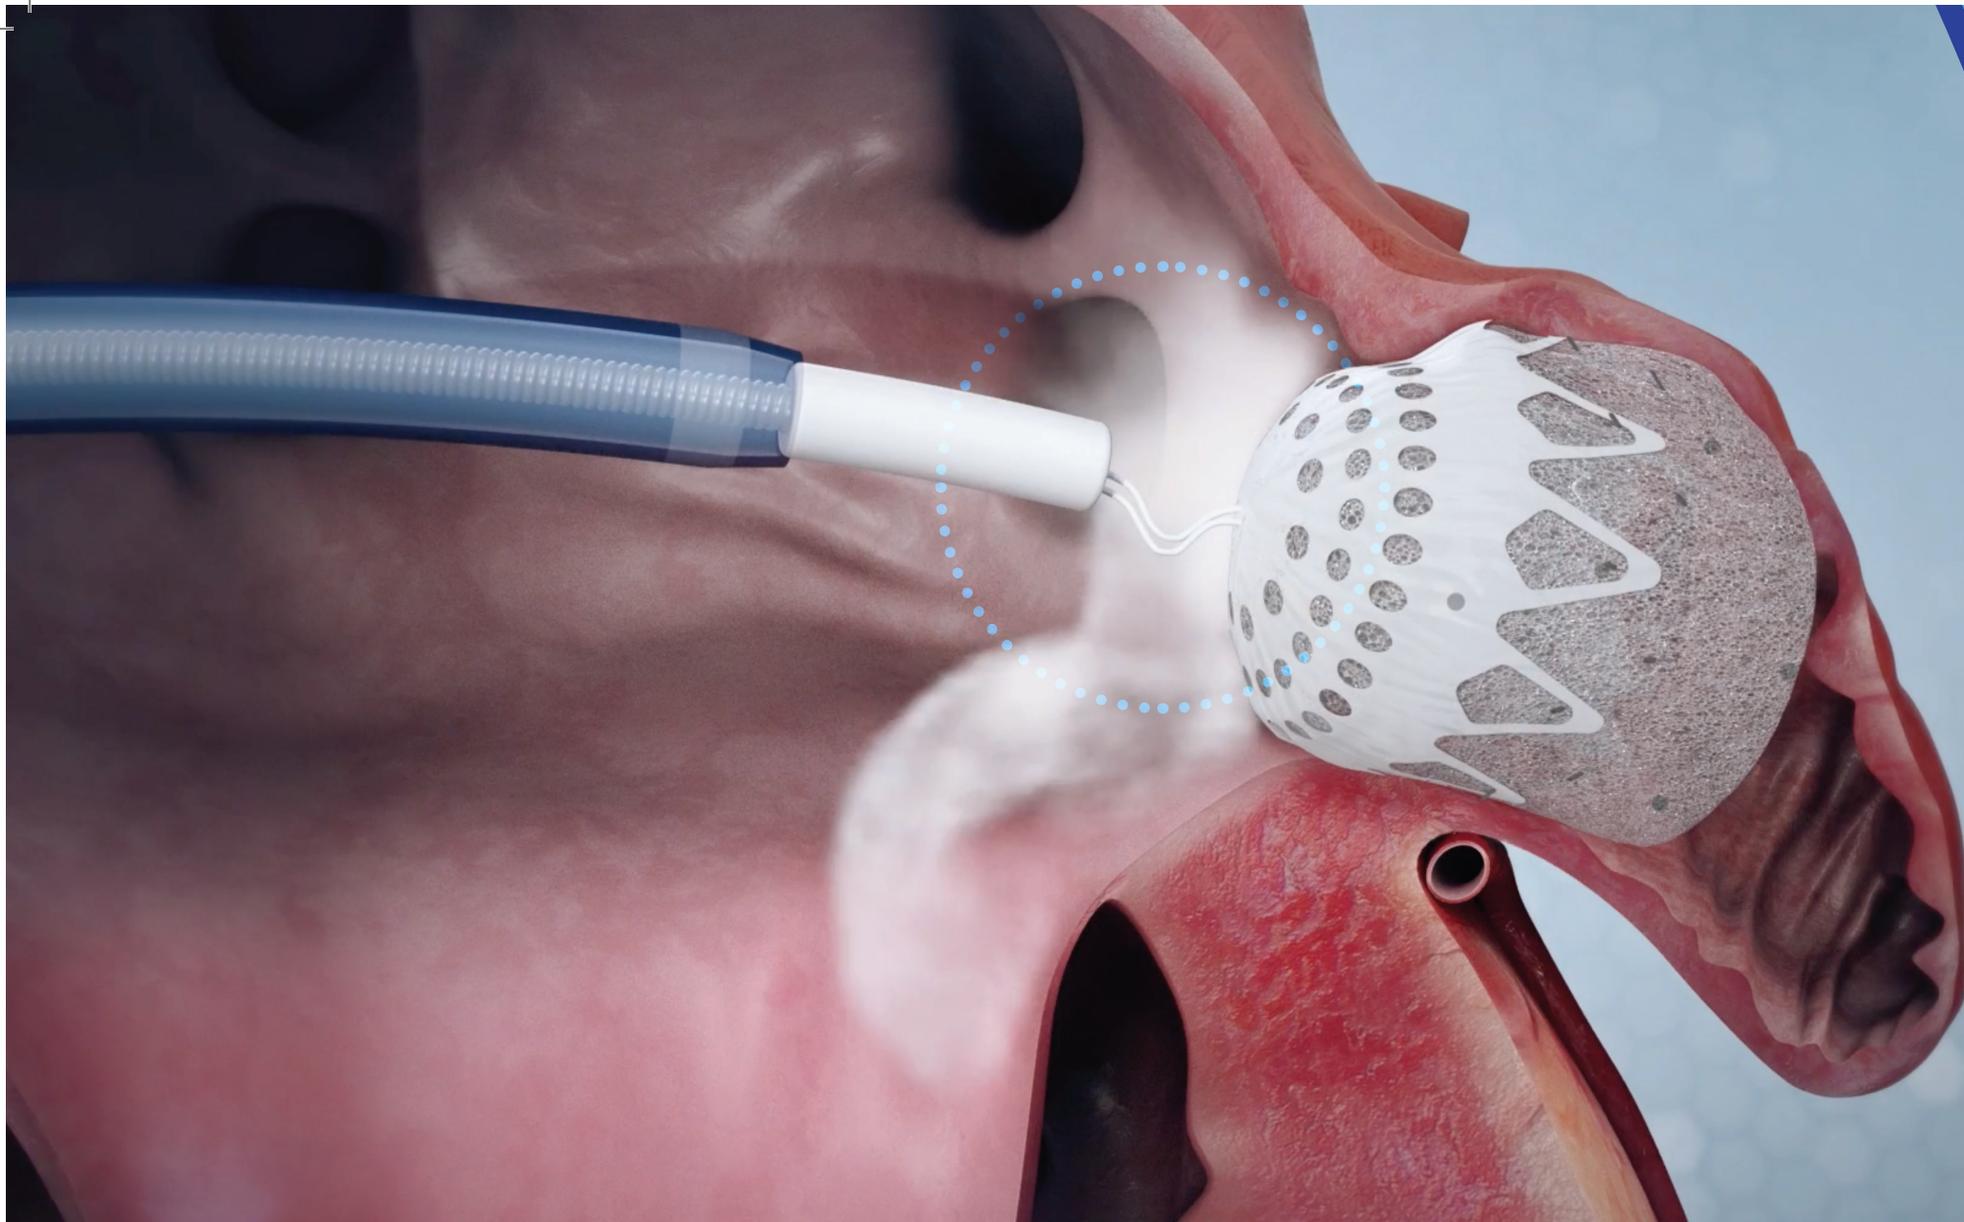


CONFORM

PIVOTAL TRIAL

Positioning Confirmed

Your doctor will take another image to confirm the implant is positioned correctly.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

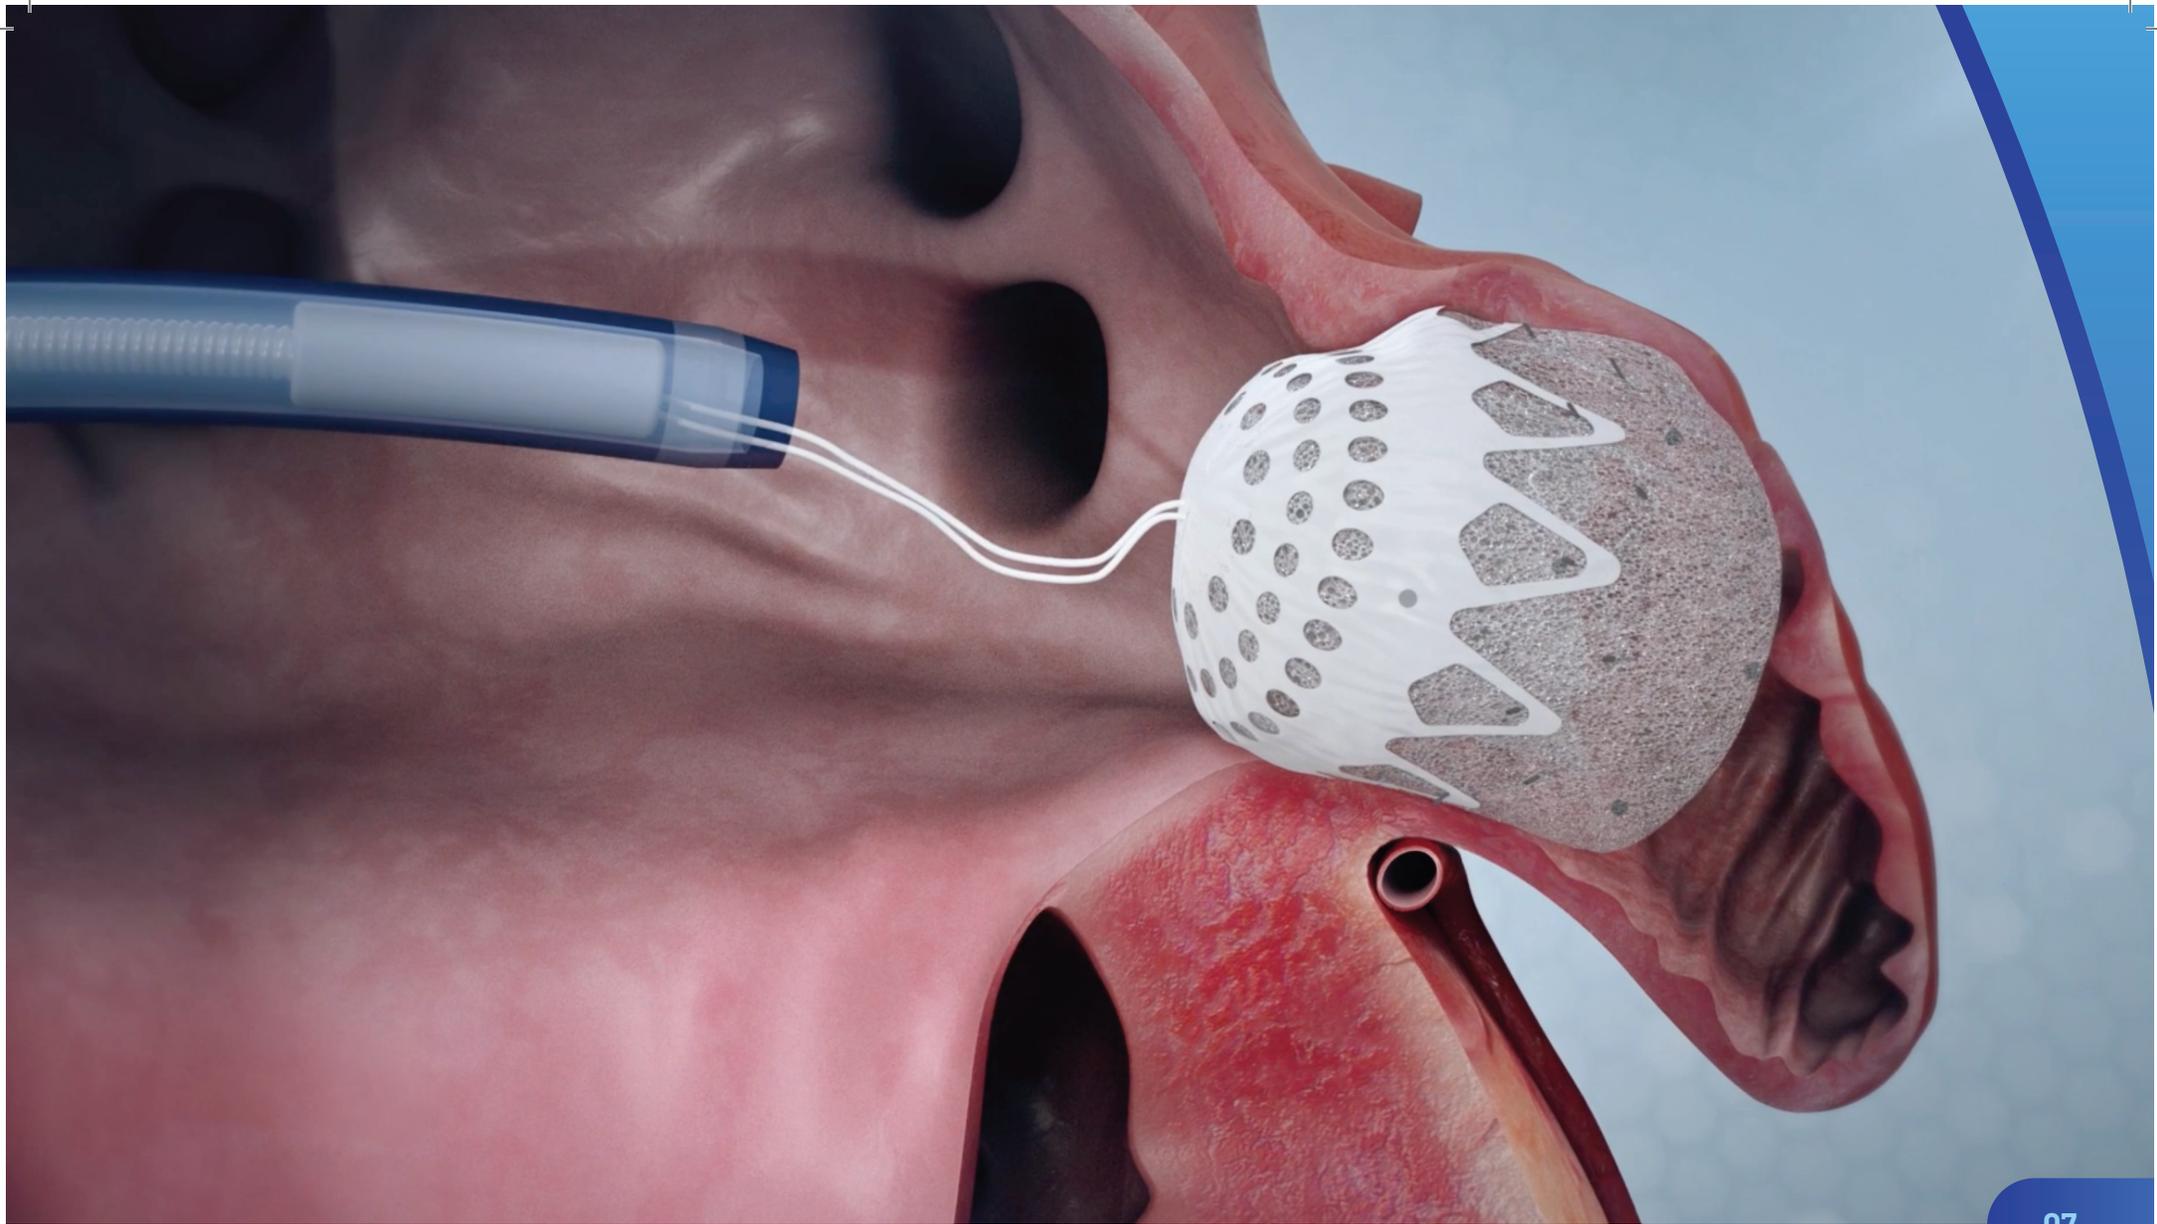


CONFORM

PIVOTAL TRIAL

Implant Release

Once proper positioning is confirmed, the implant is released from the delivery system.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

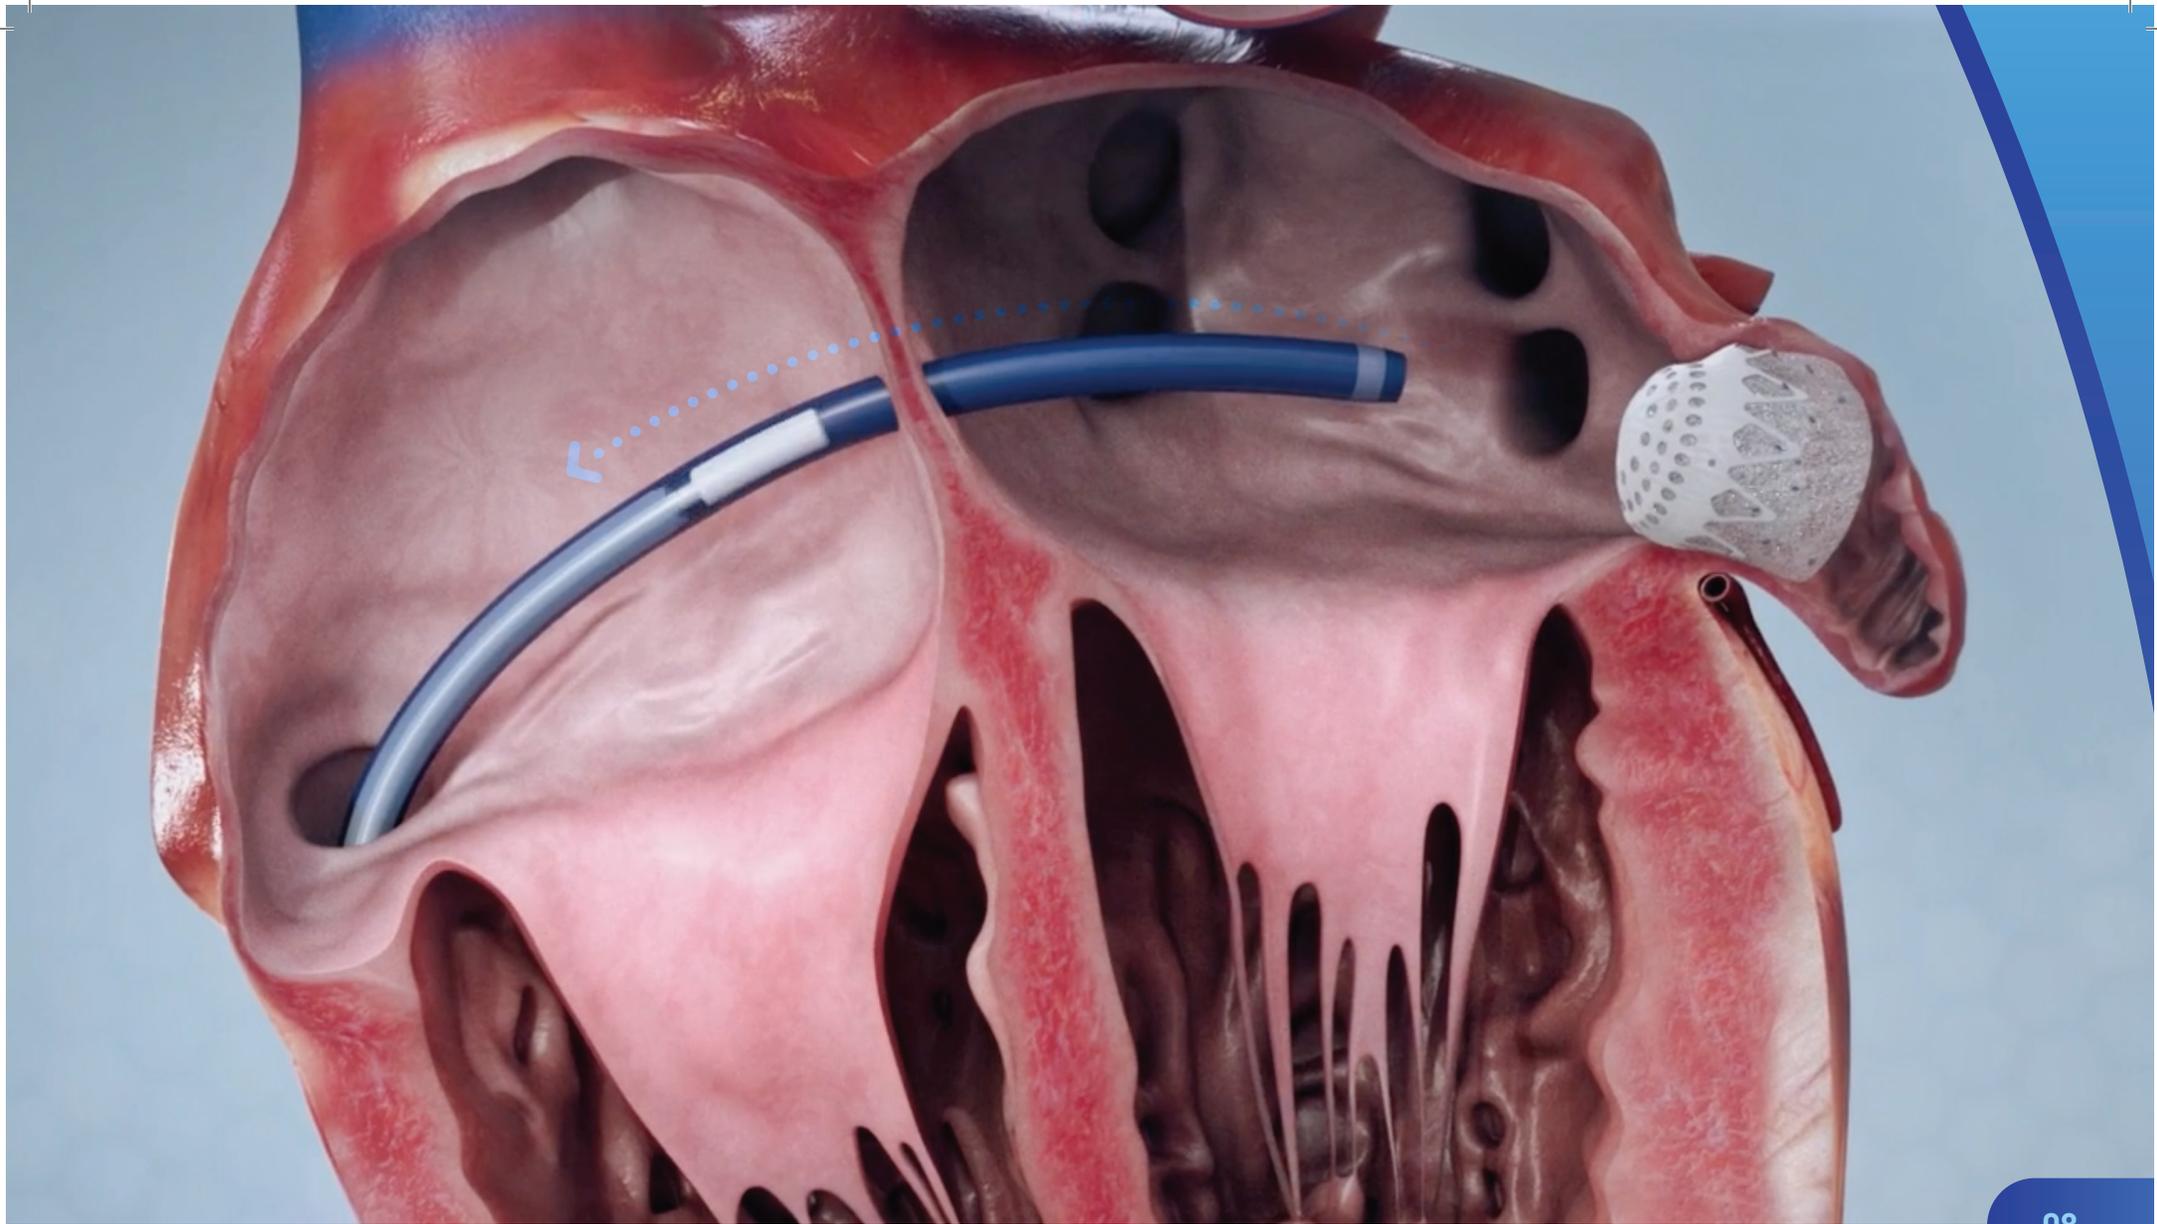


CONFORM
PIVOTAL TRIAL

Delivery System Removal

The implant remains in place to seal the appendage.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

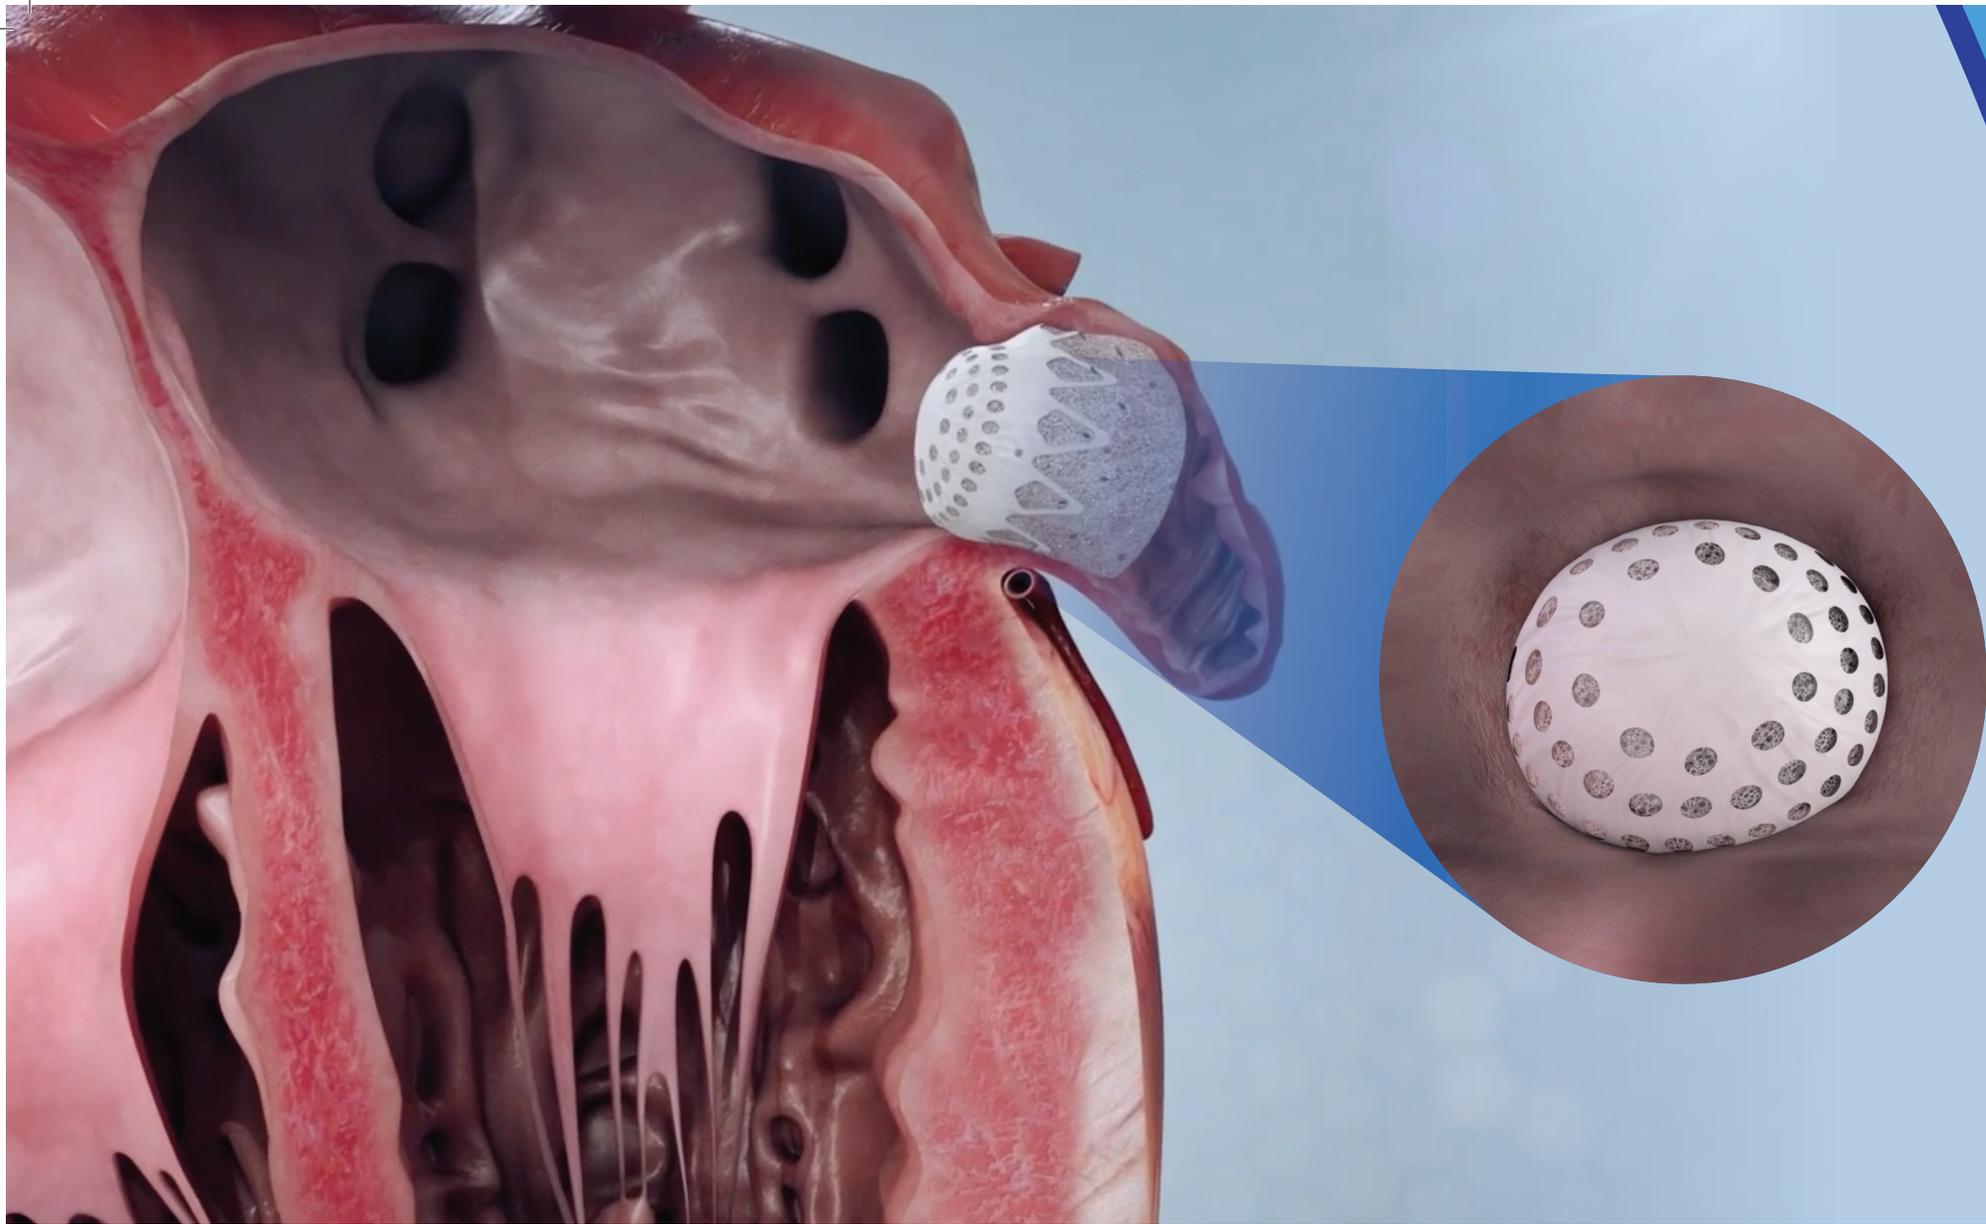

CONFORM
PIVOTAL TRIAL

Intended to Permanently Seal
With the implant in position, the procedure is complete.

CAUTION: Investigational device. Limited by United States law to investigational use only. Not available for sale.

The logo features the word "CONFORM" in a large, bold, black sans-serif font. The letter "O" is replaced by a blue circle with a white dot in the center. Below "CONFORM" is the phrase "PIVOTAL TRIAL" in a smaller, black, all-caps sans-serif font with wide letter spacing. The text is centered within a large, light gray circle that has a subtle gradient. The background of the entire slide is white, with several concentric dotted circles radiating from the center, creating a ripple effect.

CONFORM

PIVOTAL TRIAL

CAUTION: Investigational device. Limited by United States
law to investigational use only. Not available for sale.
60-00476 rev A